
Designed for above the knee interventions



BioPath 035 is indicated for:

- > De-novo lesions
- > Restenosis after realisation of balloon and /or stent PTA
- > Pre- and post-dilatation in case of peripheral stent implantation

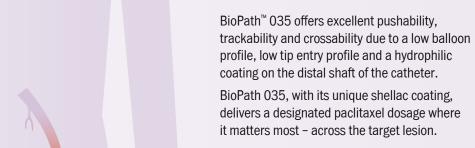

Ordering Information

Balloon diameter (mm)	Balloon length (mm)							
	20	40	60	80	100	120	150	
4.0	BPTH-35-4020 S	BPTH-35-4040 S	BPTH-35-4060 S	BPTH-35-4080 S	BPTH-35-40100 S	BPTH-35-40120 S	BPTH-35-40150 S	
	BPTH-35-4020 L	BPTH-35-4040 L	BPTH-35-4060 L	BPTH-35-4080 L	BPTH-35-40100 L	BPTH-35-40120 L	BPTH-35-40150 L	
5.0	BPTH-35-5020 S	BPTH-35-5040 S	BPTH-35-5060 S	BPTH-35-5080 S	BPTH-35-50100 S	BPTH-35-50120 S	BPTH-35-50150 S	
	BPTH-35-5020 L	BPTH-35-5040 L	BPTH-35-5060 L	BPTH-35-5080 L	BPTH-35-50100 L	BPTH-35-50120 L	BPTH-35-50150 L	
6.0	BPTH-35-6020 S	BPTH-35-6040 S	BPTH-35-6060 S	BPTH-35-6080 S	BPTH-35-60100 S	BPTH-35-60120 S	BPTH-35-60150 S	
	BPTH-35-6020 L	BPTH-35-6040 L	BPTH-35-6060 L	BPTH-35-6080 L	BPTH-35-60100 L	BPTH-35-60120 L	BPTH-35-60150 L	
7.0	BPTH-35-7020 S	BPTH-35-7040 S	BPTH-35-7060 S	BPTH-35-7080 S	BPTH-35-70100 S	BPTH-35-70120 S	BPTH-35-70150 S	
	BPTH-35-7020 L	BPTH-35-7040 L	BPTH-35-7060 L	BPTH-35-7080 L	BPTH-35-70100 L	BPTH-35-70120 L	BPTH-35-70150 L	
8.0	BPTH-35-8020 S	BPTH-35-8040 S	BPTH-35-8060 S	BPTH-35-8080 S	BPTH-35-80100 S	S: 80 cm usa	S: 80 cm usable catheter length L: 135 cm usable catheter length	
	BPTH-35-8020 L	BPTH-35-8040 L	BPTH-35-8060 L	BPTH-35-8080 L	BPTH-35-80100 L			

- 1. Axel D.L. et al. Circulation 1997; 96:636-45
- 2. A. Posa et al. Catheterization and Cardiovascular Interventions 76:395-403 (2010)
- 3. Data on file

BioPath™ 035 paclitaxel-eluting balloon catheter is CE Mark approved.

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings and instructions for use can be found in the product labeling supplied with each device.

BioPath is a trademark or registered trademark of Biosensors International Group, Ltd. All cited trademarks are the property of their respective owners.

Les informations relatives à ce produit ne sont pas destinées aux professionnels de santé exerçant en France – Any information related to this product is not intended for health care professionals who practice in France.

Not available for sale in the United States and certain other countries.
© 2014 Biosensors International Group, Ltd. All rights reserved.



BIOSENSORS EUROPE SA

Rue de Lausanne 29 1110 Morges Switzerland Tel: +41 (0)21 804 80 00

Fax: +41 (0)21 804 80 01

BIOSENSORS INTERVENTIONAL TECHNOLOGIES PTE LTD

36 Jalan Tukang Singapore 619 266 Tel: +65 6213 5777 Fax: +65 6213 5737



Latest generation paclitaxel-eluting balloon for peripheral interventions

the right reach



The right reach

The treatment process

With balloon dilatation, the injuries to the arterial wall initiate an inflammatory reaction with an excretion of growth factors which trigger the onset of cell division and smooth muscle cell migration.

Paclitaxel prevents restenosis by stabilizing microtubal formation and thus prevents the cells going through the phases of replication, resulting in the inhibition of cell division.

Paclitaxel reduces the excretion of the platelet derived growth factor (PDGF) that mediates vascular smooth muscle cell migration to the intima1.

Hydrophilic shaft coating


. .

The BioPath™ 035 balloon coating

- > The BioPath 035 balloon coating consists of a 1:1 mixture of paclitaxel (3 μg/mm²) and shellac, a natural resin approved by the FDA (GRAS), and by Europe (E904) as a food additive.
- ▶ BioPath 035 delivers the designated concentration of paclitaxel locally to the arterial tissue.
- The properties of shellac protect the paclitaxel during transition and placement.

Delivering the drug

Once in contact with blood, the shellac and paclitaxel coating swells and begins to open, facilitating the pressure-induced transfer of the paclitaxel.






Delivering the paclitaxel drug

Immediately after the controlled PTA, injury to the vessel wall key pathways contribute to the formation of neointimal hyperplasia. Injury from cracking plaque can lead to narrowing of the lumen.

The paclitaxel dose will act over the short term to inhibit cell re-growth.

- Pre-dilatation prepares the way for the delivery of paclitaxel from the
- BioPath 035 is advanced to the lesion site.
- Once the operator is satisfied with the position of BioPath 035 across the lesion, an inflation at 6 bar for at least 60 seconds will deliver the paclitaxel through the cracked plaque and onto the vessel wall.
- BioPath 035 is then withdrawn. The shellac carrier remains on the balloon surface.



Designed for above the knee interventions

Over-the-wire (OTW) catheter Inflation/deflation lumen Separate guide wire lumen **Low Tip Entry Profile**

A choice of balloon length and diameter, on two catheter shaft lengths

30 sec

Coronary² and **Peripheral**³ –

20 sec

Tissue paclitaxel levels 45 minutes post-dilatation

45 sec (n=7)

Available balloon diameters 4.0, 5.0, 6.0, 7.0 and 8 mm Balloon lengths 20, 40, 60, 80, 100, 120 and 150 mm S: 80 cm or L: 135 cm Usable catheter lengths

60 sec

0.035"

Recommended guide wire

For illustration purpose only - not to scale.